

Clinical Laboratory Test Update

Trichomonas vaginalis testing update


- Effective 2/22/2017, the University of Colorado Hospital Clinical Laboratory will offer two new tests for Trichomonas vaginalis testing on cervical, vaginal, male or female urine, and male urethral specimens collected by the appropriate GenProbe Aptima device (see table below and picture for examples).
- Trichomonas culture (LAB8614 and LAB3446) will be discontinued.

NEW TESTS:

Test Names	1) TRICHOMONAS GENPROBE (LAB8918) 2) CHLAMYDIA/GC/TRICH GENPROBE (LAB8915)
Collection device	GenProbe Aptima Unisex swab (endocervical and male urethral specimens) GenProbe Aptima Urine Collection Kit (male and female urine specimens) GenProbe Aptima Vaginal Swab Specimen Collection Kit (vaginal specimens) ESWABS WILL NOT BE ACCEPTED.
Performed	Mon - Fri
Turnaround Time	Same day received, next run if repeat testing is necessary

APPROPRIATE COLLECTION DEVICES currently available at UCHealth.

- Urine collection tube (top)
- Unisex collection swab for cervical or male urethral specimens (bottom)
- ESwabs will NOT be accepted

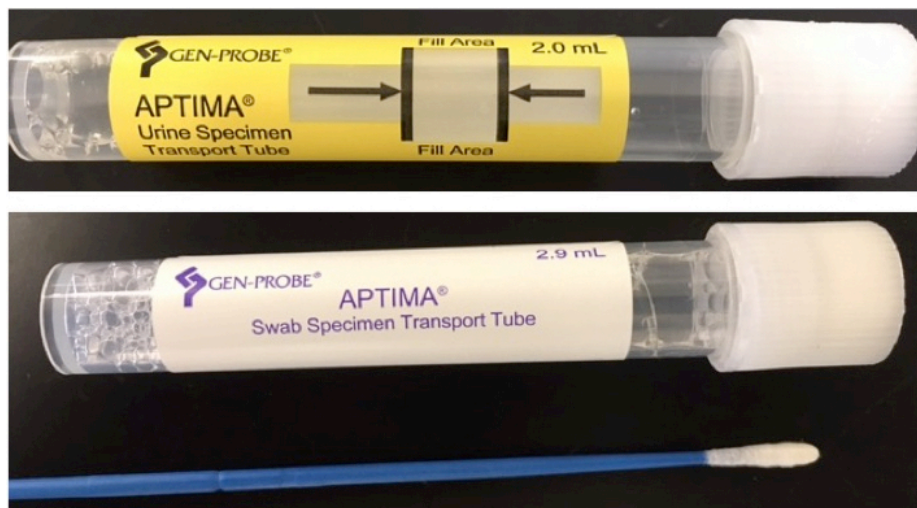

Please call the University of Colorado Hospital Clinical Laboratory Molecular Diagnostics Department at 720-848-6892 if you have any questions or visit our test catalog at <https://www.testmenu.com/universityhospital> for further information.

Issued: 02/15/2017